



Makrolon® Rx2430

PC

Covestro Deutschland AG

- MVR (300 °C/1.2 kg) 19 cm³/10 min
- medical devices
- suitable for sterilization with high-energy radiation
- biocompatible according to many ISO 10993-1 test requirements
- low viscosity
- transparent parts for medical devices

Rheological properties	Value	Unit	Test Standard
ISO Data			
Melt volume-flow rate, MVR	19	cm³/10min	ISO 1133
Temperature	300	°C	-
Load	1.2	kg	-
Molding shrinkage, parallel	0.6	%	ISO 294-4, 2577
Molding shrinkage, normal	0.7	%	ISO 294-4, 2577

Mechanical Properties	Value	Unit	Test Standard
ISO Data			
Tensile Modulus	2400	MPa	ISO 527
Yield stress	67	MPa	ISO 527
Yield strain	6.1	%	ISO 527
Nominal strain at break	>50	%	ISO 527
Impact Strength (Charpy), +23°C	no break	kJ/m²	ISO 179/1eU
Impact Strength (Charpy), -30°C	no break	kJ/m²	ISO 179/1eU
Puncture - maximum force, +23°C	5300	N	ISO 6603-2
Puncture - maximum force, -30°C	6200	N	ISO 6603-2
Puncture energy, +23°C	60	J	ISO 6603-2
Puncture energy, -30°C	70	J	ISO 6603-2

Thermal Properties	Value	Unit	Test Standard
ISO Data			
Temp. of deflection under load (1.80 MPa)	122	°C	ISO 75-1/-2
Temp. of deflection under load (0.45 MPa)	134	°C	ISO 75-1/-2
Vicat softening temperature, 50°C/h 50N	141	°C	ISO 306
Coeff. of Linear Therm. Expansion, parallel	65	E-6/K	ISO 11359-1/-2
Coeff. of Linear Therm. Expansion, normal	65	E-6/K	ISO 11359-1/-2
Burning Behav. at thickness h	V-2	class	UL 94
Thickness tested	0.4	mm	-

Electrical Properties	Value	Unit	Test Standard
ISO Data			
Volume Resistivity	>1E13	Ohm*m	IEC 62631-3-1
Surface Resistivity	>1E15	Ohm	IEC 62631-3-2

Other Properties	Value	Unit	Test Standard
ISO Data			
Water Absorption	0.3	%	Sim. to ISO 62
Humidity absorption	0.12	%	Sim. to ISO 62
Density	1200	kg/m³	ISO 1183

Test specimen production	Value	Unit	Test Standard
ISO Data			
Injection Molding, melt temperature	280	°C	ISO 294
Injection Molding, mold temperature	80	°C	ISO 294
Injection Molding, injection velocity	200	mm/s	ISO 294

Processing Recommendation Injection Molding	Value	Unit	Test Standard
Pre-drying - Temperature	120	°C	-
Pre-drying - Time	2 - 3	h	-
Processing humidity	≤0.02	%	-
Melt temperature	280 - 320	°C	-
Mold temperature	80 - 100	°C	-


Makrolon® Rx2430

PC


Covestro Deutschland AG

Diagrams

Viscosity-shear rate

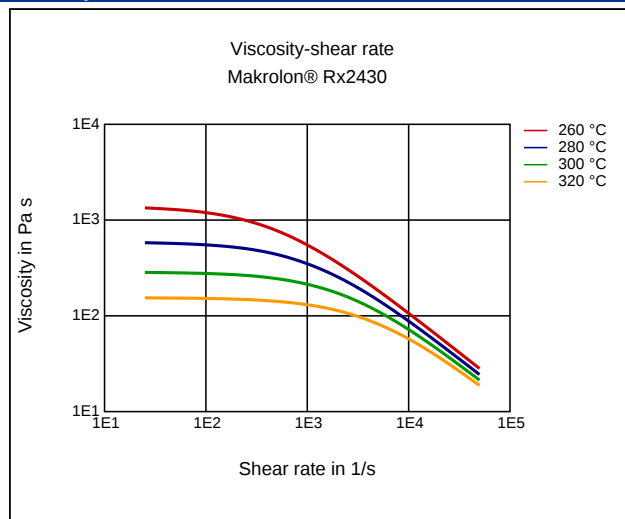

Shearstress-shear rate

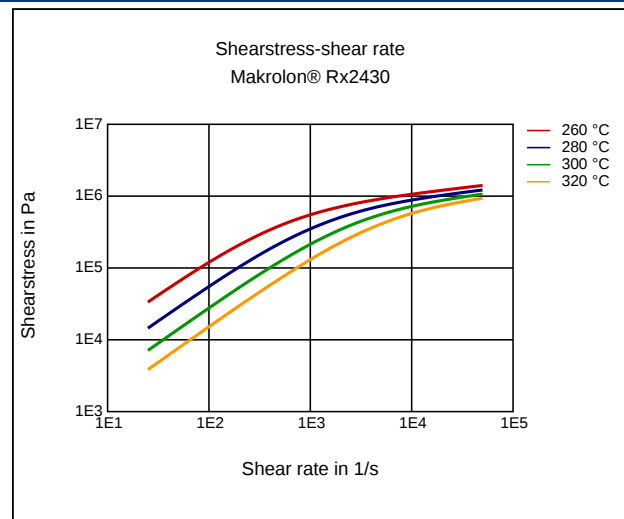

Characteristics

Processing

Injection Molding

Delivery form

Pellets

Special Characteristics

Transparent, Sterilizable, Ethylene Oxide (EtO) Sterilization, Steam sterilization, Gamma irradiation sterilization

Certifications

Medical, Biocompatibility ISO 10993, US Pharmacopeia Class VI Approved

Applications

Medical

Injection Molding

PREPROCESSING

Max. Water content: 0.01 - 0.02 %

Drying temperature: 120 °C

Drying time:

Circulating air drying oven (50 % fresh air) 4-8 h

Fresh air dryer (high speed dryer) 2-4 h

Dry air dryer 2-3 h

PROCESSING

Melt temperature: 280-320 °C

Mold temperature: 80-100 °C

Use open nozzle.